

TEST REPORT



Report No. : 19-065795-02-2

Page of Pages : (1) / (2)



1. Client

Name : JOIN Medical Co., Ltd.

Address : 143-40, 3F, #302 Gangdong-gu, Gangdong-daero, Seoul Korea.

Date of Receipt : 2019. 10. 08.

2. Use of Report : For submission of government office

3. Test Sample

Description : Air sterilizer

Manufacturer : NOVAERUS (Ireland) Ltd.

Model Name : NV-1050

Serial Number : ***

Remark : ***

4. Date of Test : 2019. 10. 18. ~ 2019. 10. 19.

5. Location of Test :

KTL Permanent Test (Address : 87, Digital-ro 26-gil, Guro-gu, Seoul, KOREA)

On Site Testing



6. Test Standard/Method : KOUVA AS 02 : 2019

7. Test Results : Refer to the attached results

Note : 1. This report is limited to samples submitted by the applicant and is prohibited from being used for legal or other reasons of dispute.

2. This document is valid only in its original document, and any reproduced copies and electronic copies are not valid. ("Original" means all the reports provided by the KTL including the security procedures.)

3. You can check the contents of the report by scanning the 2D Barcode below. The identity of original reports can be checked in the "Confirm original report" window of the customer's homepage (customer.ktl.re.kr).

Affirmation	Tested by Name : Park seo-hyun	 (Signature)	Technical Manager Name : JEON, Yong-Woo	 (Signature)
-------------	-----------------------------------	--	--	--

2019. 10. 22.

Korea Testing Laboratory

87, Digital-ro 26-gil, Guro-gu, Seoul, KOREA Tel.+82-2-860-1139 Fax. +82-2-860-1689

FP204-03-06



※ 위 마크는 추후 전자확인증 대조 프로그램에서 원본대조시 사용되는 2D코드입니다.

Test Results

1. Test Results

	Reference value	Results
Air sterilizer	over 60 %	98.8 %


2. Test sample

- (1) Manufacturer : NOVAERUS (Ireland) Ltd.
- (2) Model name : NV-1050
- (3) Serial number : ***

3. Test Method and Conditions

Test method	Conditions					
	Virus	Temp.	Humidity	Test time	Test Chamber	Air flow
KOUVA AS 02 : 2019	Phi-X174 (ATCC 13706-B1)	(23 ± 2) °C	(50 ± 5) % R.H.	30 minute	60 m ³	Maximum

4. Unit Photograph

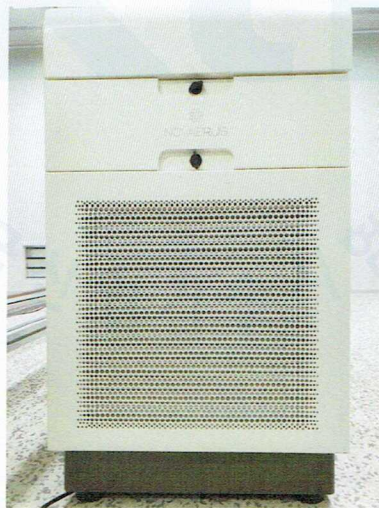

- End of document -

